
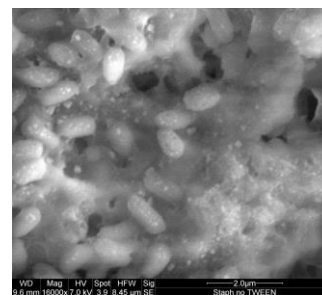
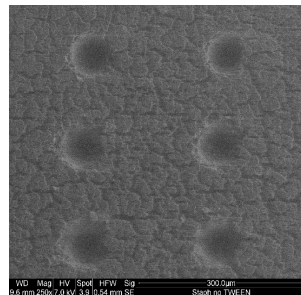


Bacterial Limit of Detection Reduction Utilizing a Novel Sample Preparation Protocol


Steven J. Rehse, Jeremy Marvin, Alexandra E. Paulick,
Emma Blanchette, Sydney Sleiman

Department of Physics, University of Windsor, Windsor, Ontario, Canada

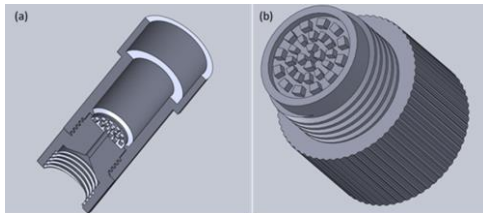


University
of Windsor

2005-2011



How unique is "unique"?

✓ We can identify a bacterial species, certainly its genus, with high sensitivity and

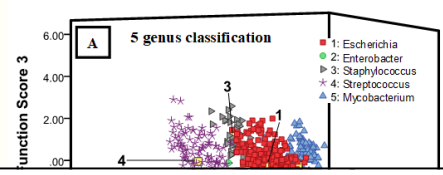

Spectrochimica Acta Part B 154 (2019) 50-69

8 publications in Spectroscopy



Contents lists available at ScienceDirect

Spectrochimica Acta Part B

journal homepage: www.elsevier.com/locate/sab



Invited Review


A review of the use of laser-induced breakdown spectroscopy for bacterial classification, quantification, and identification

Steven J. Rehse*


University of Windsor, Department of Physics, Windsor, Ontario N9B 3P4, Canada

DFA: Sensitivity: 91.37 ± 16.39 % Specificity: 97.46 ± 9.35 %
PLSDA: Sensitivity: 93.13 ± 10.25 % Specificity: 90.60 ± 21.33 %

2011-2019



Can we develop this to be a convenient and easy-to-use (for clinicians) test?




Early days (at Wayne State)

Advantages:

- ✓ Background free mounting substrate

Disadvantages:

- X Not really flat
- X Degrades
- X Hard to make
- X Watery

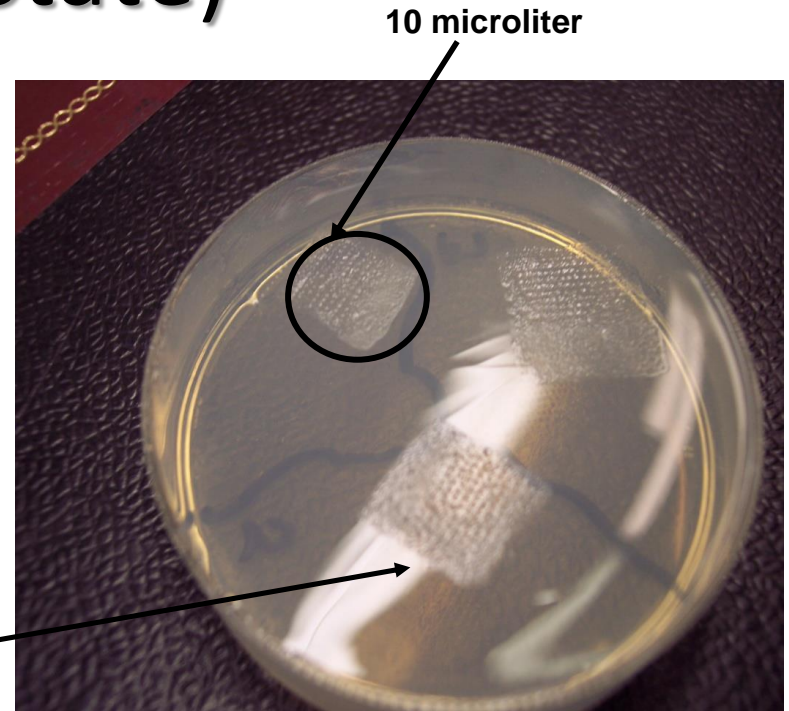


10 microliter

about 500-1500
bacteria per
sampling location


Nutrient-free bacto-agar



Moving to Filters (Early Days at Windsor)

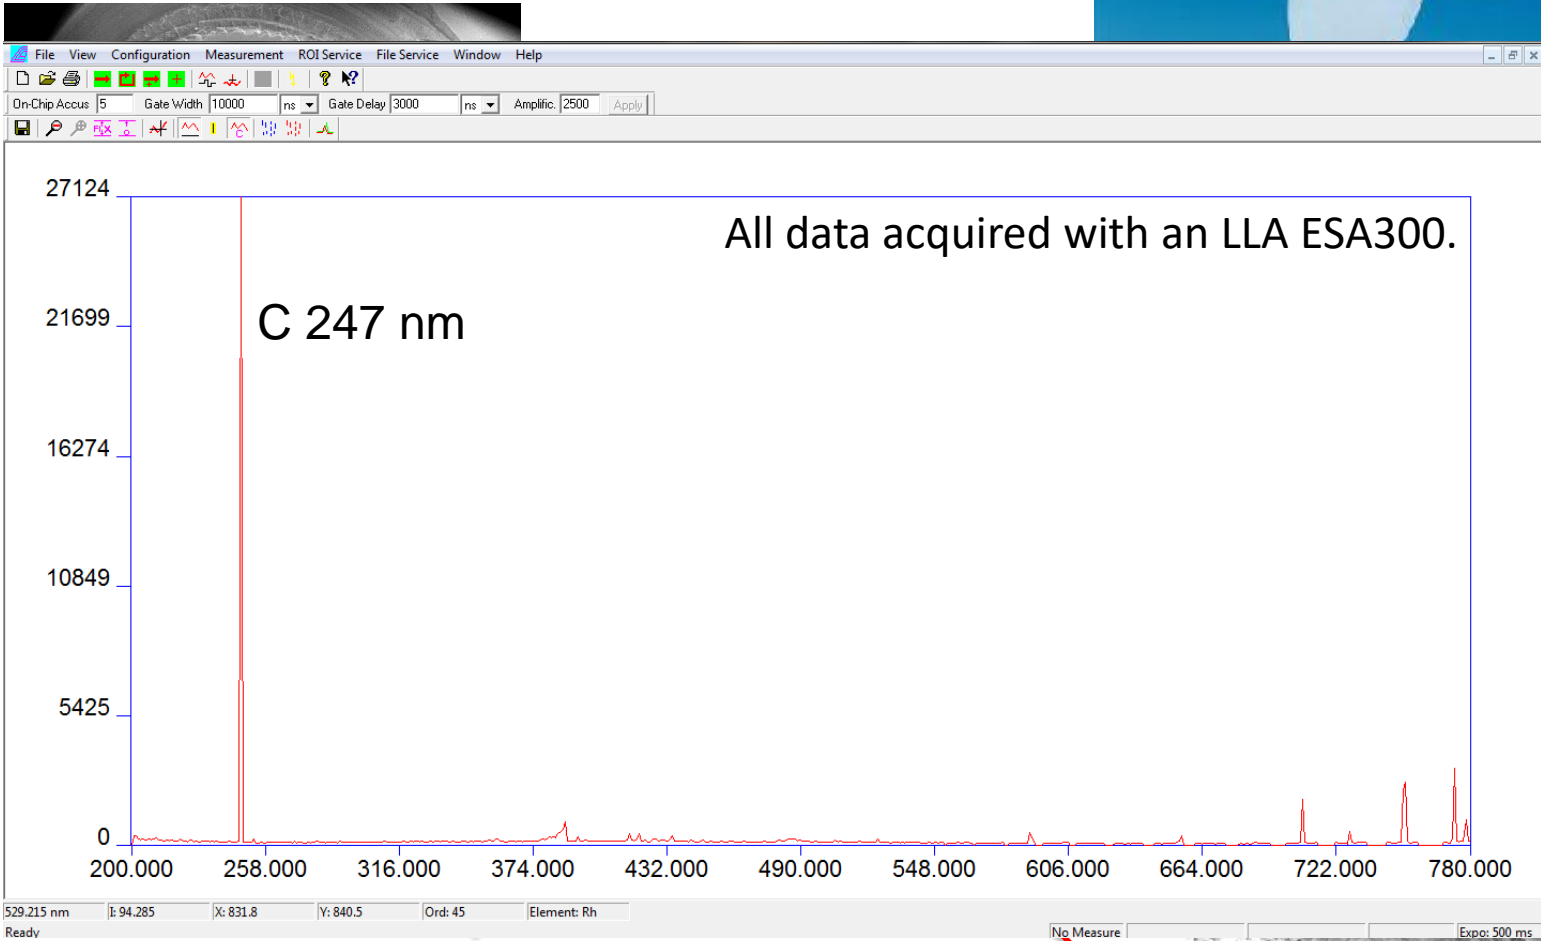


lters

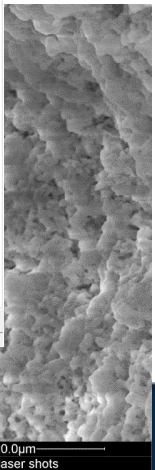

How to get bacteria onto filters?




How to get bacteria onto filters?

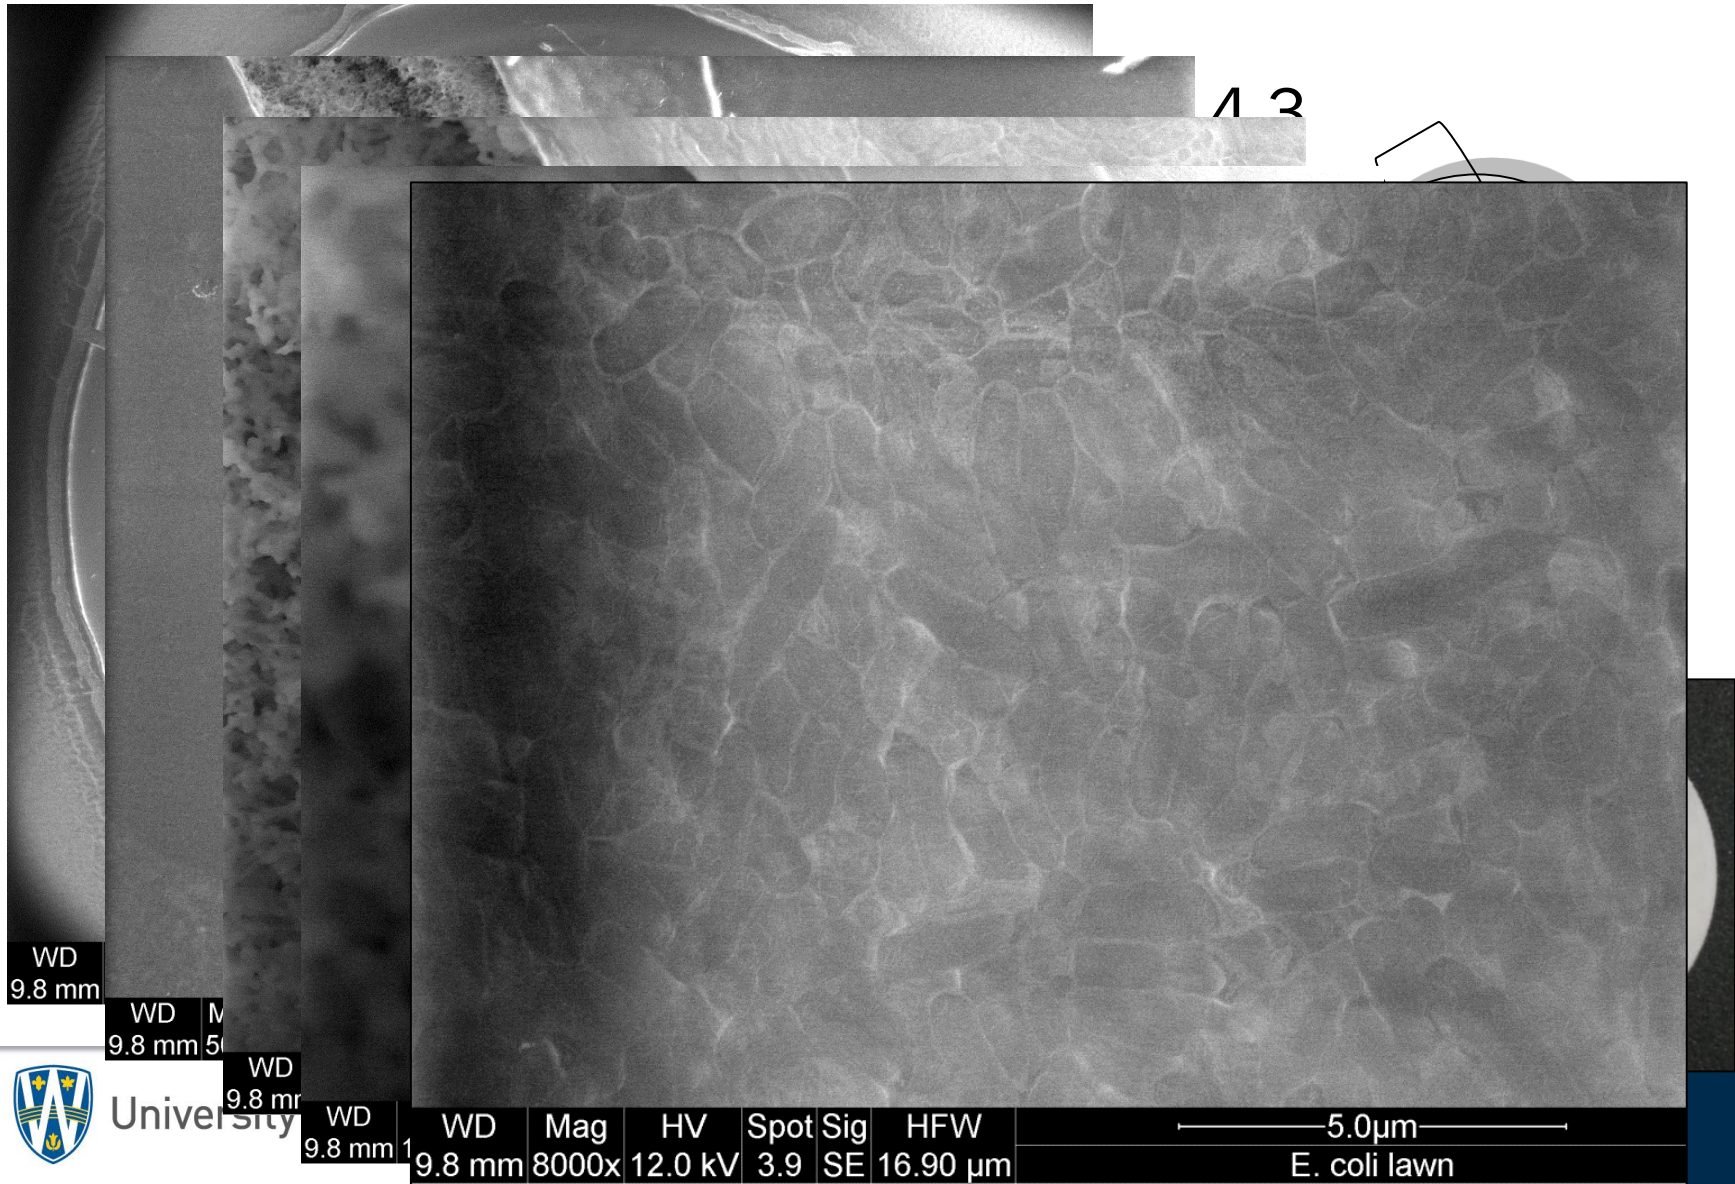


Typical bacterial LIBS spectrum

Currently: using matched parabolic reflectors into fiber for UV

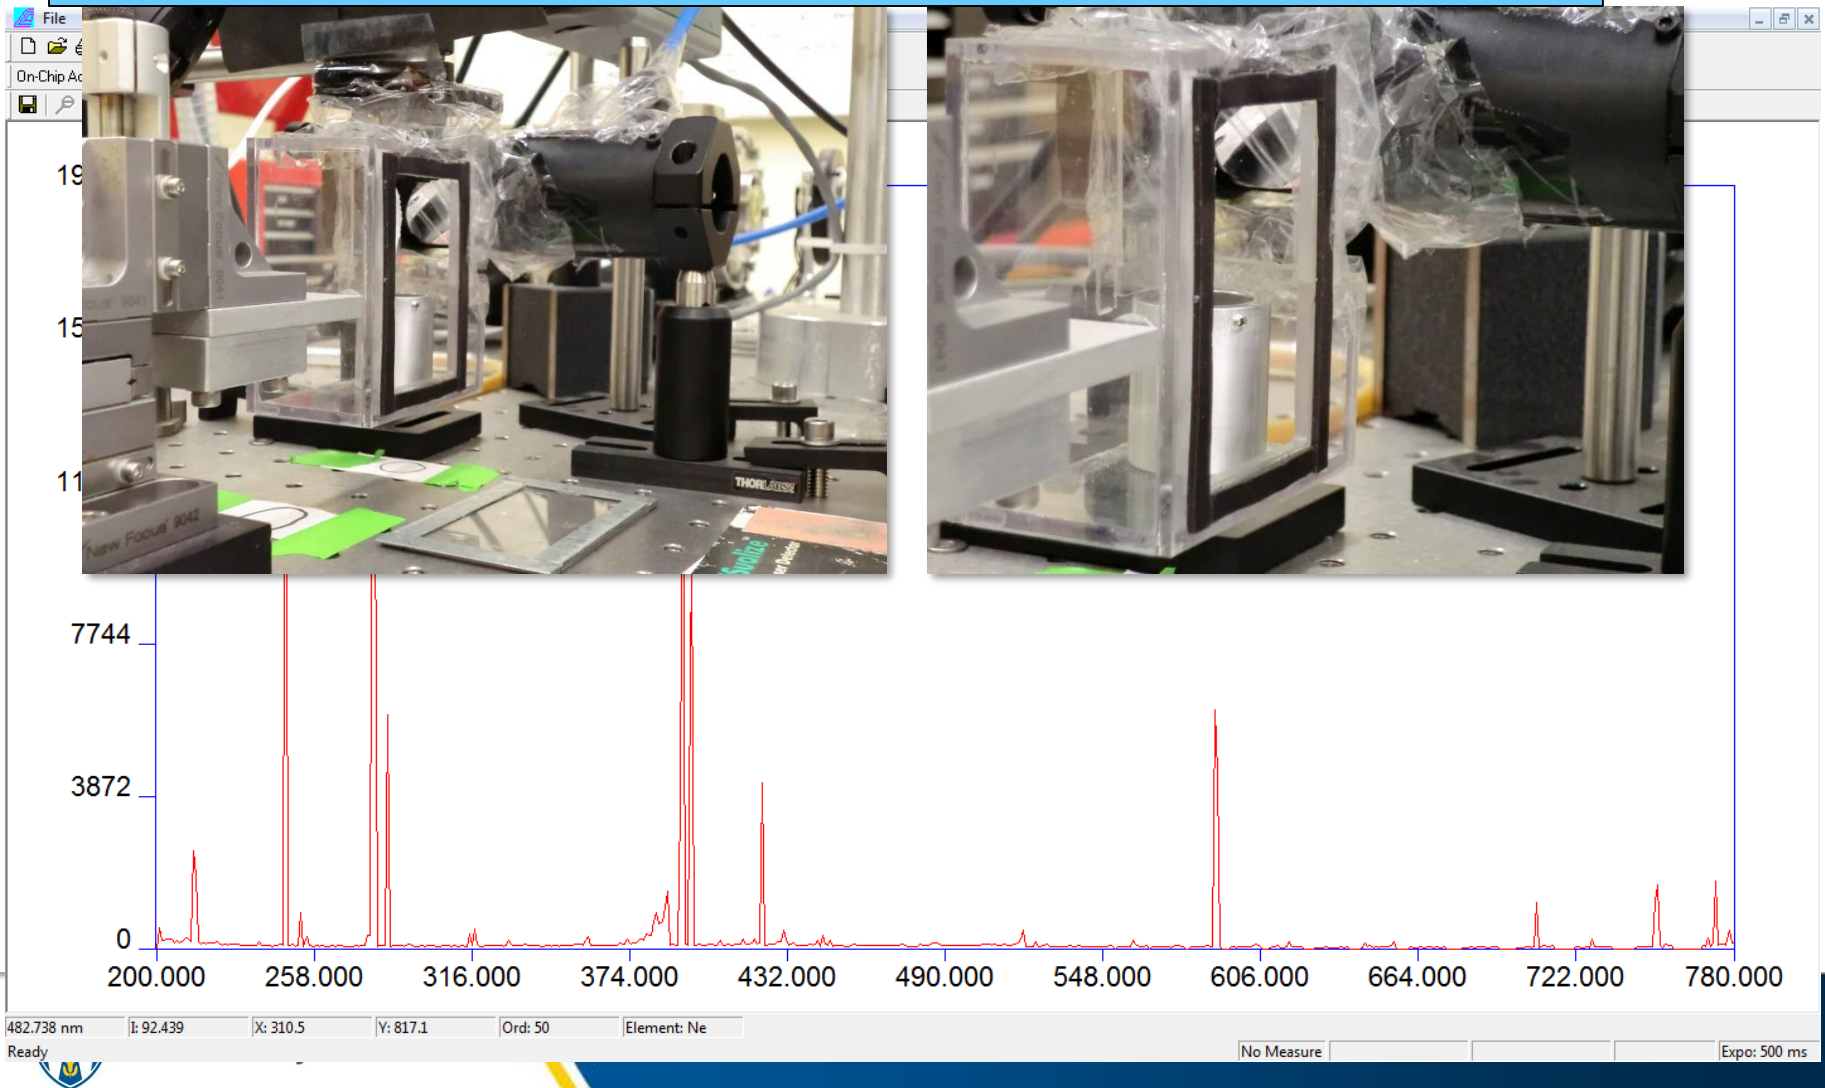


Data analysis with variable down selection

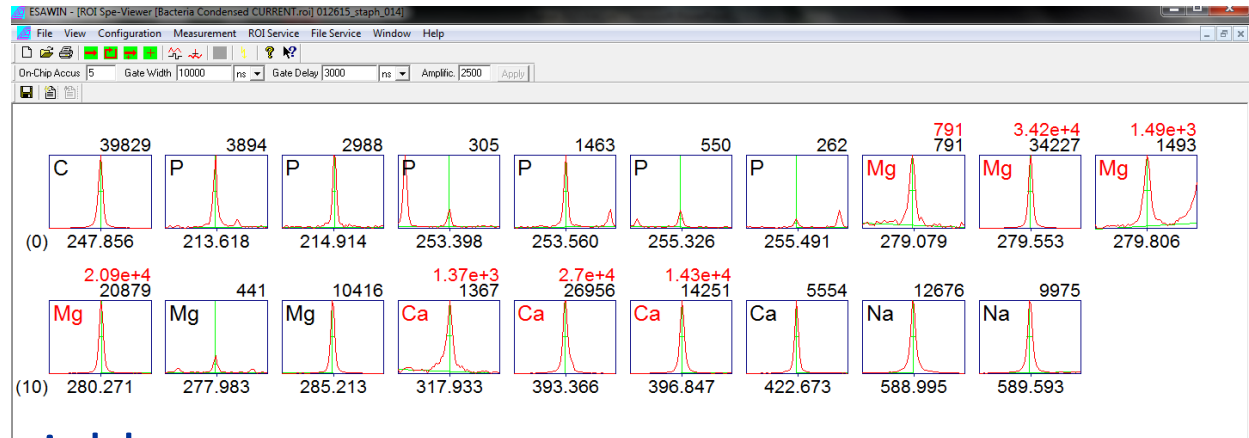

- 164 independent variables
 - 19 line intensities (all divided by sum)
 - 145 ratios of intensities



Performance on filters

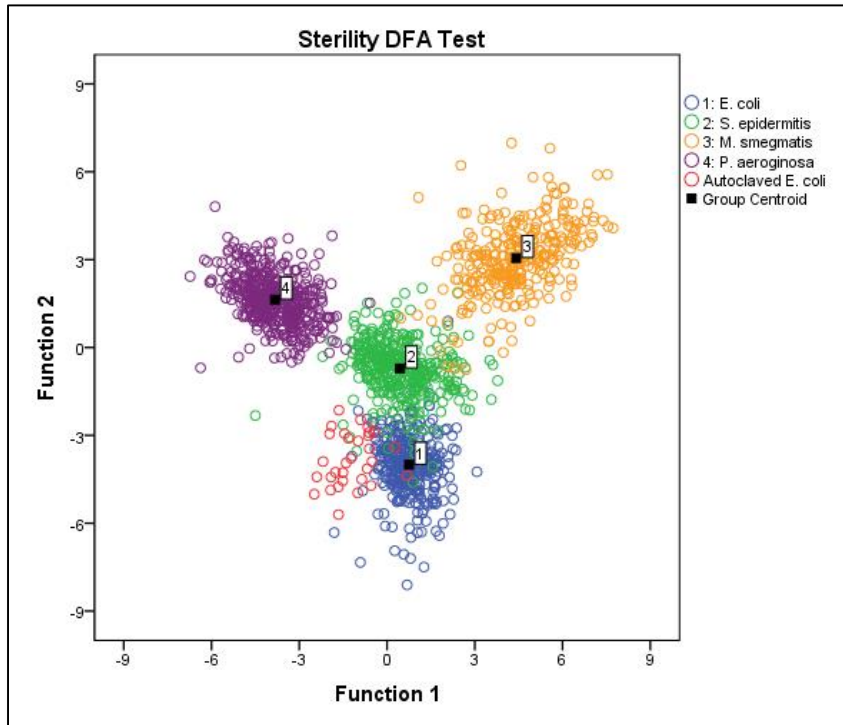

DFA Classification Grouped by Species

Escherichia	TRUE	FALSE	Staphylococcus	TRUE	FALSE
Positive	98.28%	0.77%	Positive	97.75%	1.44%
Negative	99.23%	1.72%	Negative	98.56%	2.25%
Mycobacterium	TRUE	FALSE	Pseudomonas	TRUE	FALSE
Positive	95.36%	0.33%	Positive	99.57%	0.22%
Negative	99.67%	4.64%	Negative	99.78%	0.43%

Sensitivity: 98 ± 2% Specificity: 99 ± 1%

PLS-DA Classification Grouped by Species

Escherichia	TRUE	FALSE	Staphylococcus	TRUE	FALSE
Positive	96.55%	1.12%	Positive	96.75%	1.53%
Negative	98.88%	3.45%	Negative	98.47%	3.25%
Mycobacterium	TRUE	FALSE	Pseudomonas	TRUE	FALSE
Positive	97.02%	0.41%	Positive	98.92%	0.33%
Negative	99.59%	2.98%	Negative	99.67%	1.08%





Sensitivity: 97 ± 3% Specificity: 99 ± 2%

All external validation results

	DFA (by filter)	DFA (by species) above	PLSDA (by species) above
Sensitivity	0.93±0.07	0.98±0.02	0.97±0.03
Specificity	0.98±0.03	0.99±0.01	0.99±0.02




Using filters, a better way: the centrifuge insert

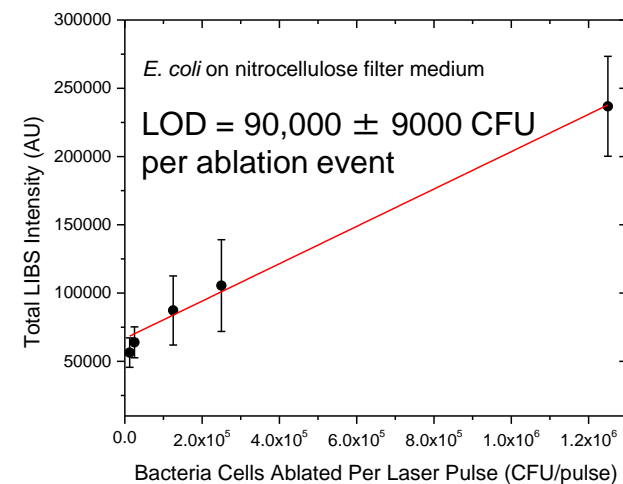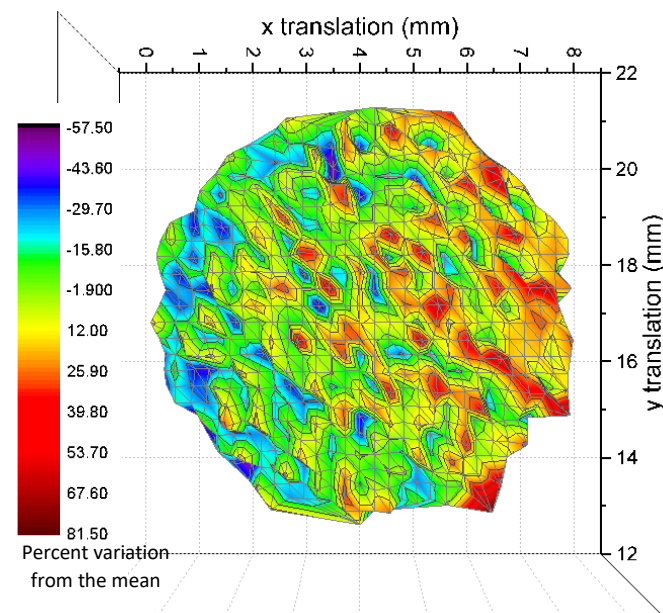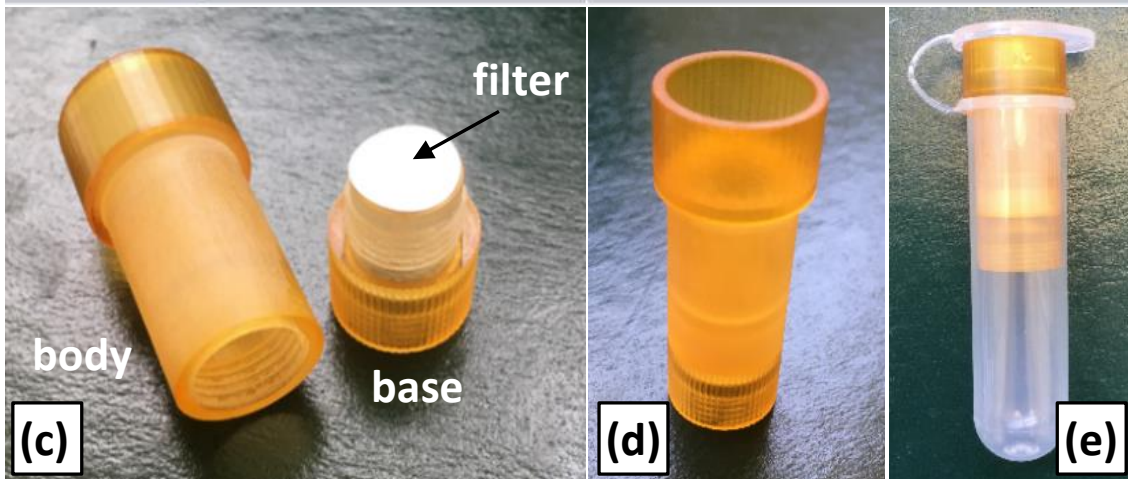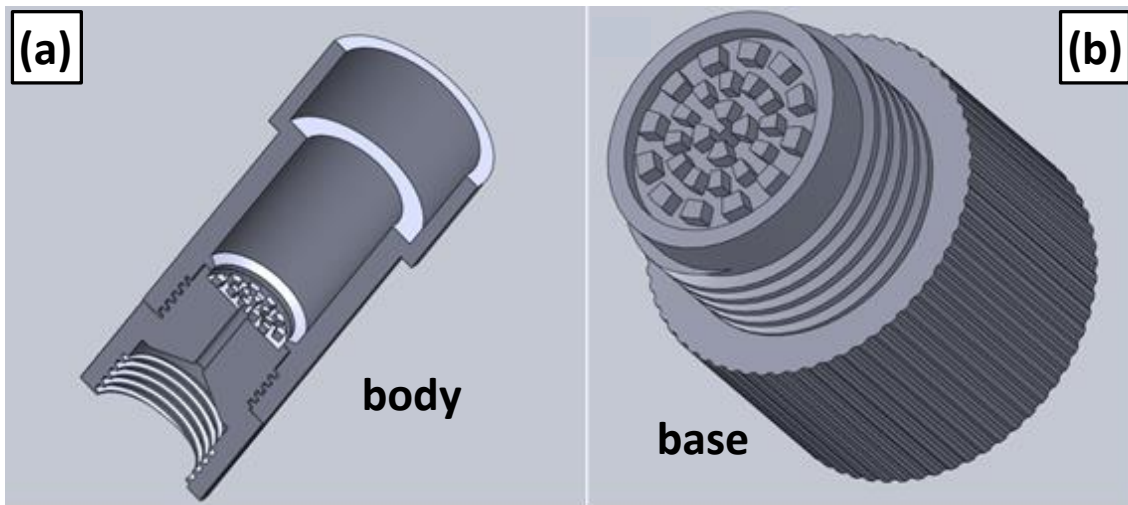

The centrifuge insert for cell sorting

Tungsten powder
average particle
size of 12 μm
used to sterilize
contaminated

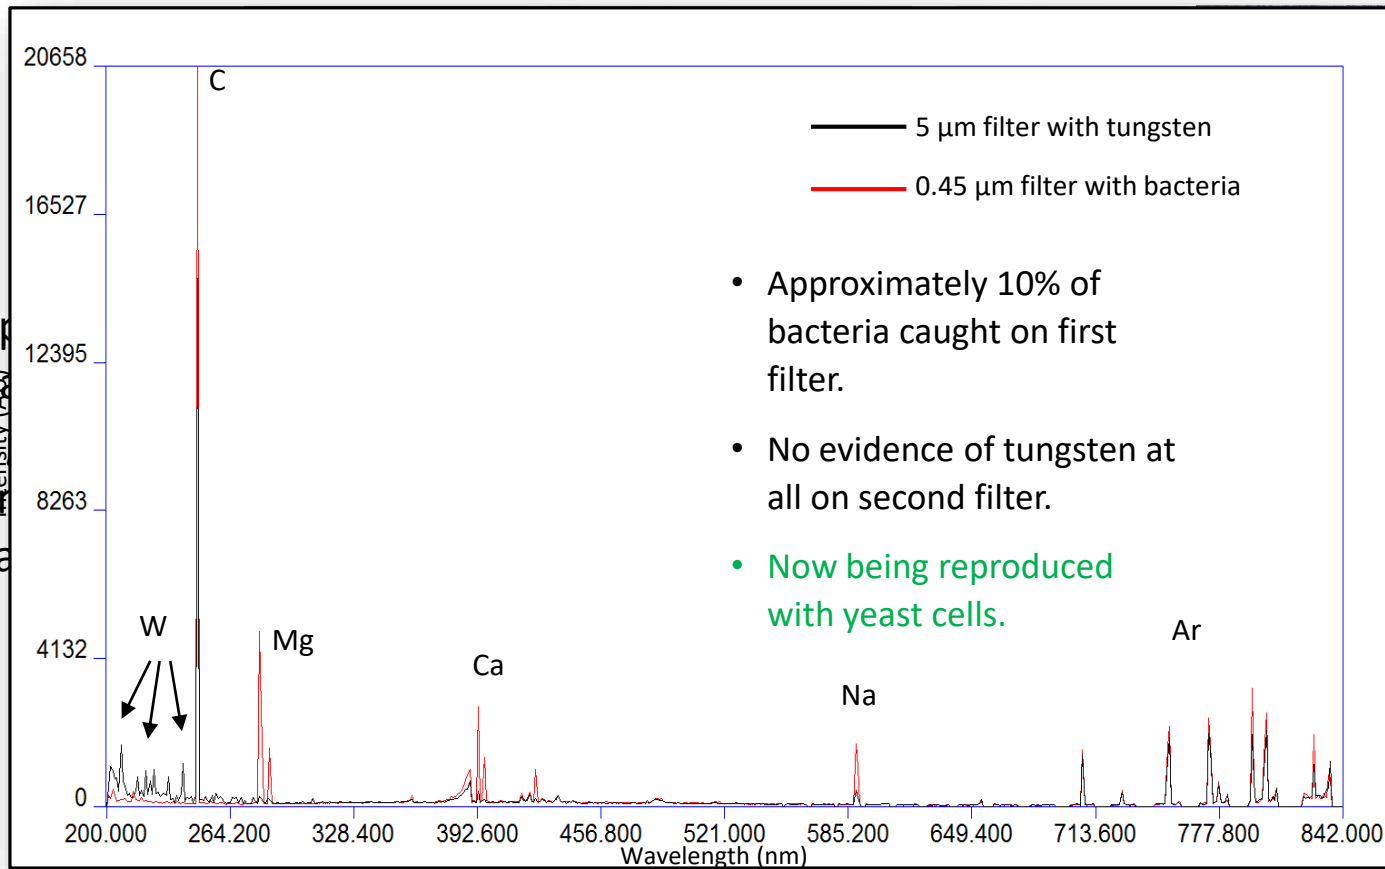

- Tungsten powder was chosen for its inertness, cost and availability, safety of use, ease of preparation, biologically relevant size, and elemental purity.
- Tungsten powder was added to a suspension of *E. coli*, vortexed, and ~ 0.1 mL was pipetted into the top of the insert prior to centrifugation.




Using filters, a better way: the centrifuge insert



Using filters, an even better way: the centrifuge cone

19 mm long Al cone

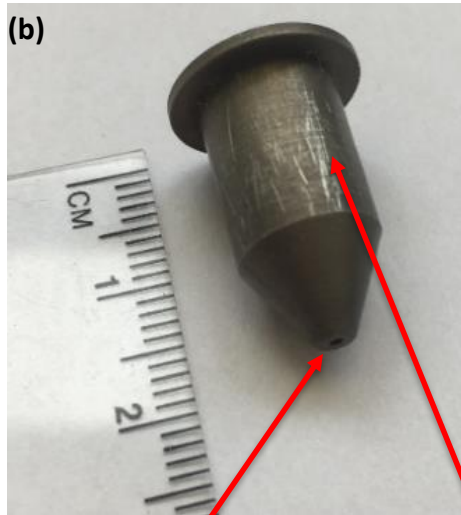

Centrifuge tube cap presses
cone into filter





1 mm hole at apex

Holds 1 mL of fluid







Cone vertex press fit into filter




Using filters, an even better way: the centrifuge cone

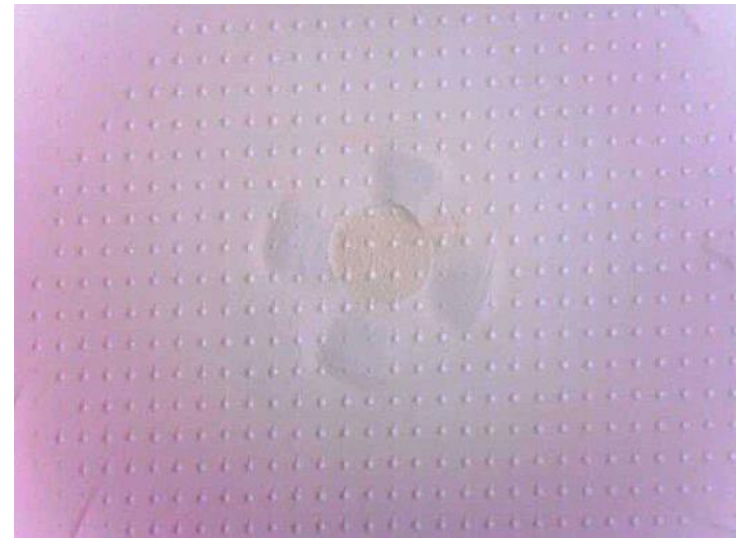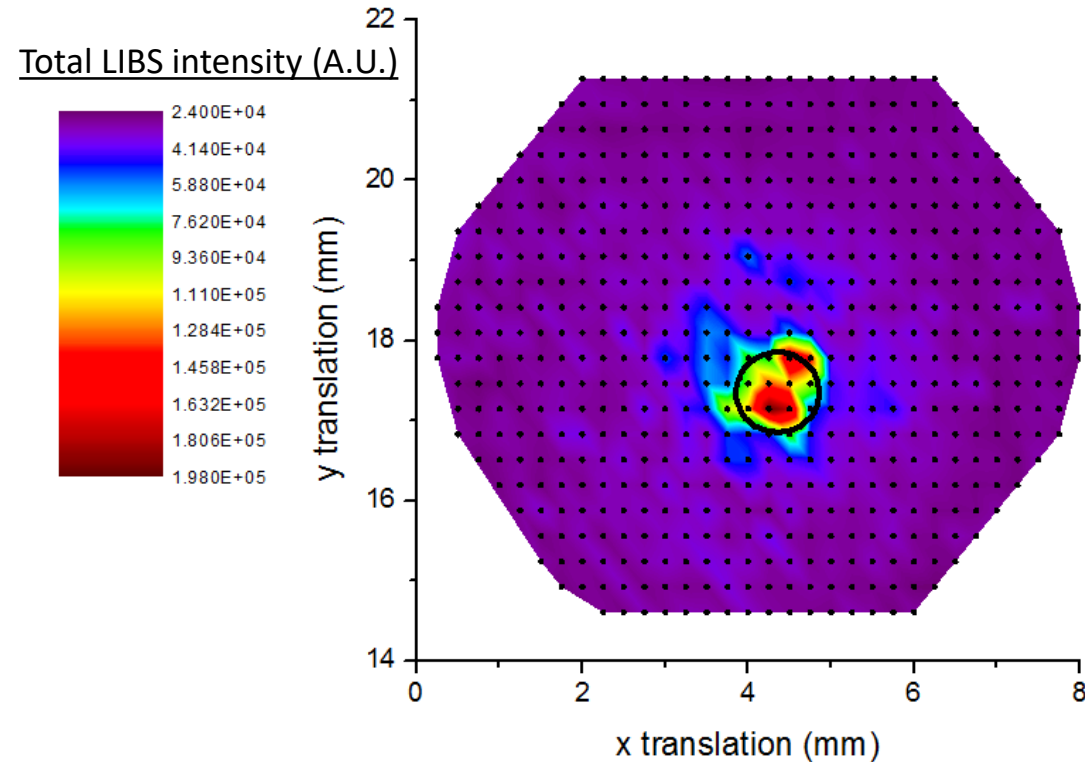

SEM micrographs

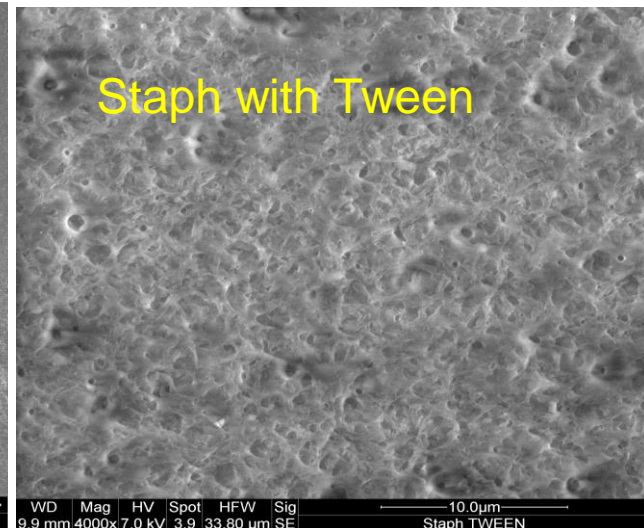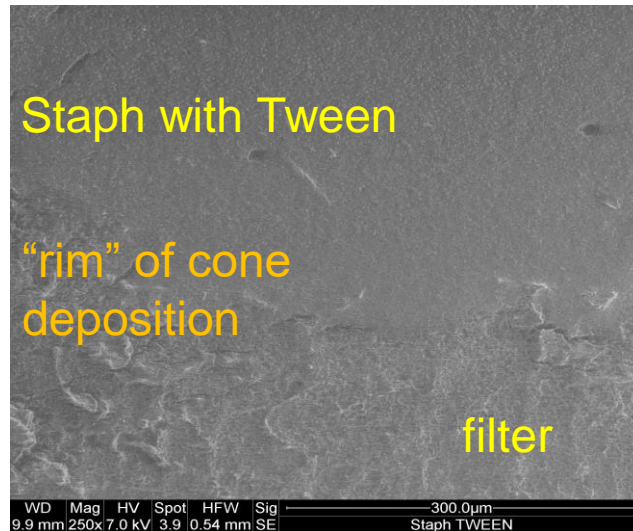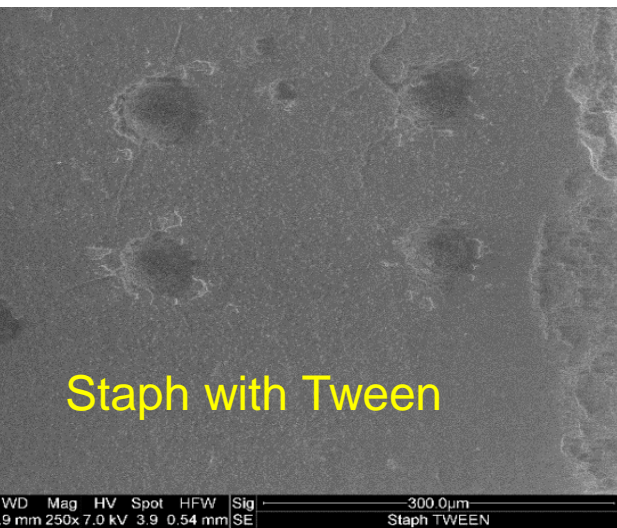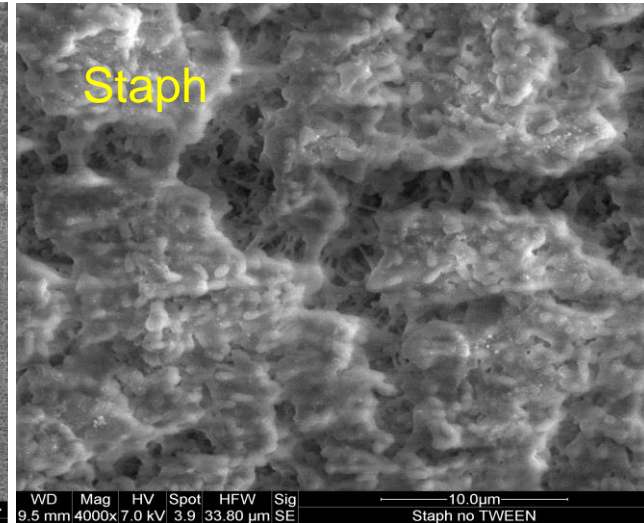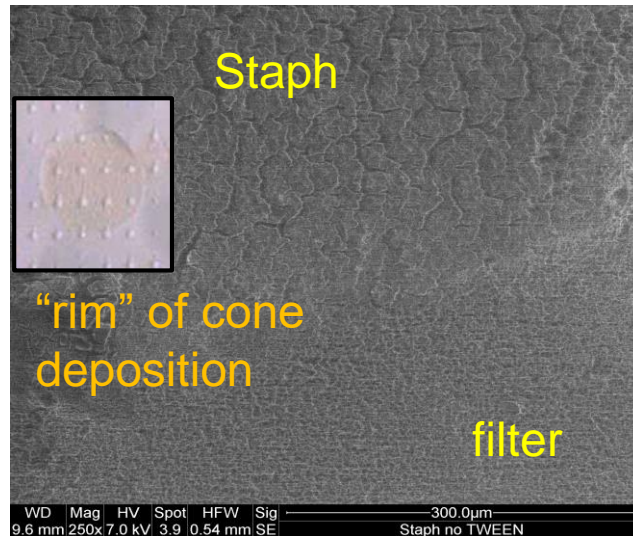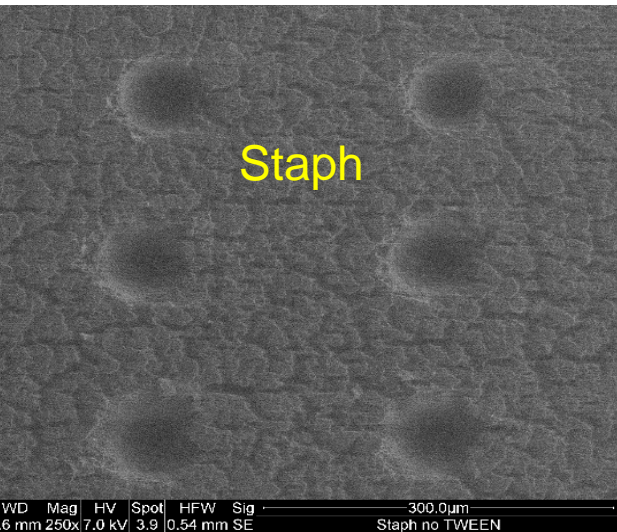

Using filters, an even better way: the centrifuge cone

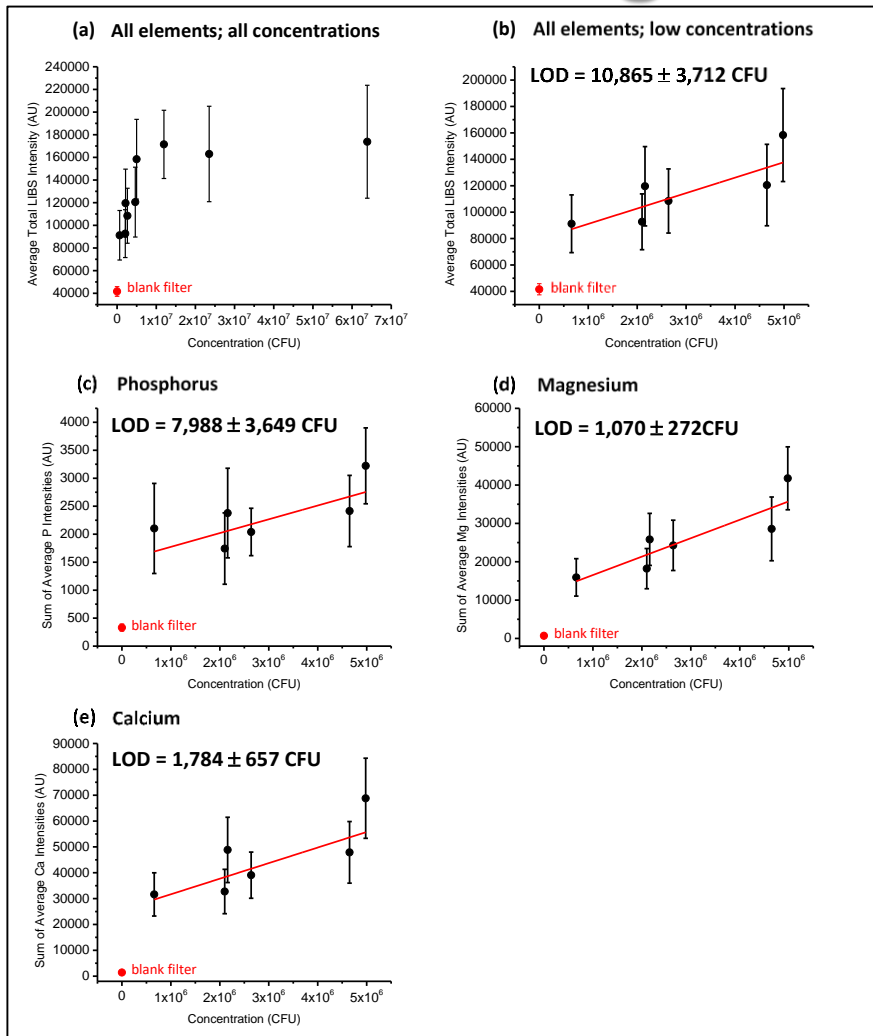

A calibration curves constructed from forty spectra obtained from each of nine different concentrations.

LIBS bacterial limit of detection of $10,865 \pm 3,712$ CFU per laser ablation event for bacteria deposited on filters using the metal cone.

LOD's calculated using only certain elements observed in the LIBS spectra and present in very low concentrations in the filter were even lower:

$1,070 \pm 272$ CFU for magnesium
 $1,784 \pm 657$ CFU for calcium.

LOD on filter better, but number of cells required in fluid specimen is **WAY** lower!





Collecting on swabs

So little bacterial sample is needed that our specimens are all collected from clinical flocked swabs.


The swab was tested for traces of contamination and did not contribute to background emission.



Deposit 100 μL of bacteria suspended in DI water onto metal plate and heat for 2 min and 20 s.

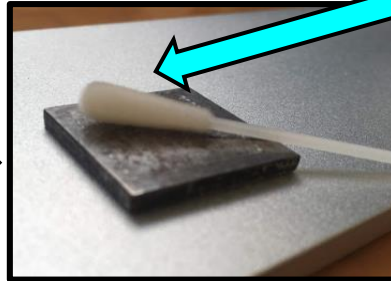


Deposit 10 μL water onto swab tip and swab metal plate.





Place swab in centrifuge tube with 1 mL of water and vortex tube for 15 s. Discard swab.



Deposit the 1 mL of sample from vortexed tube into cone, place insert into clean centrifuge tube. Centrifuge insert at 5000 rpm, 2500 g's for 5 min

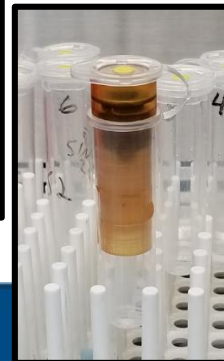

Collecting on swabs

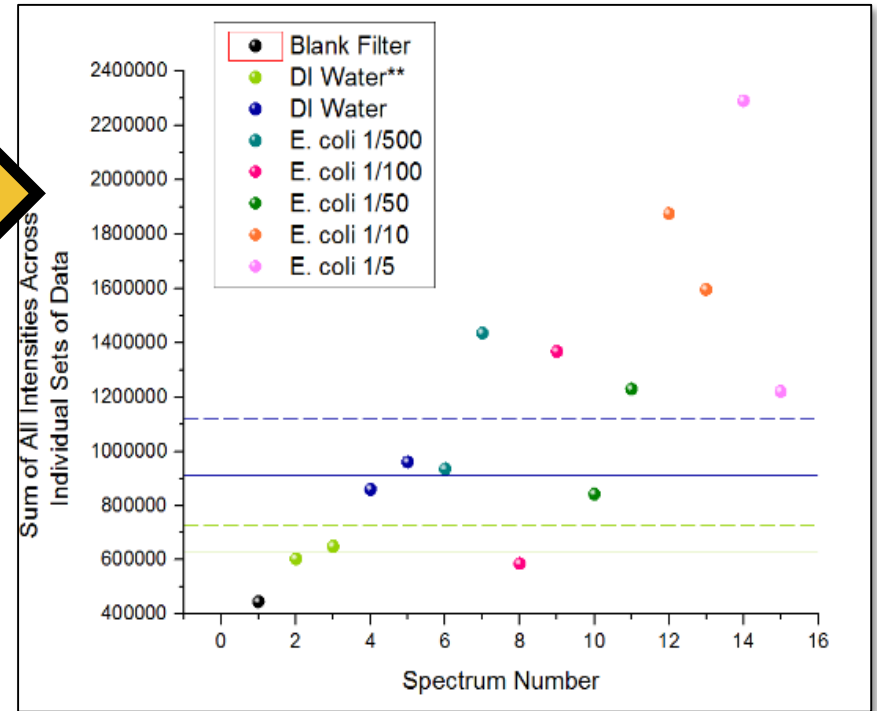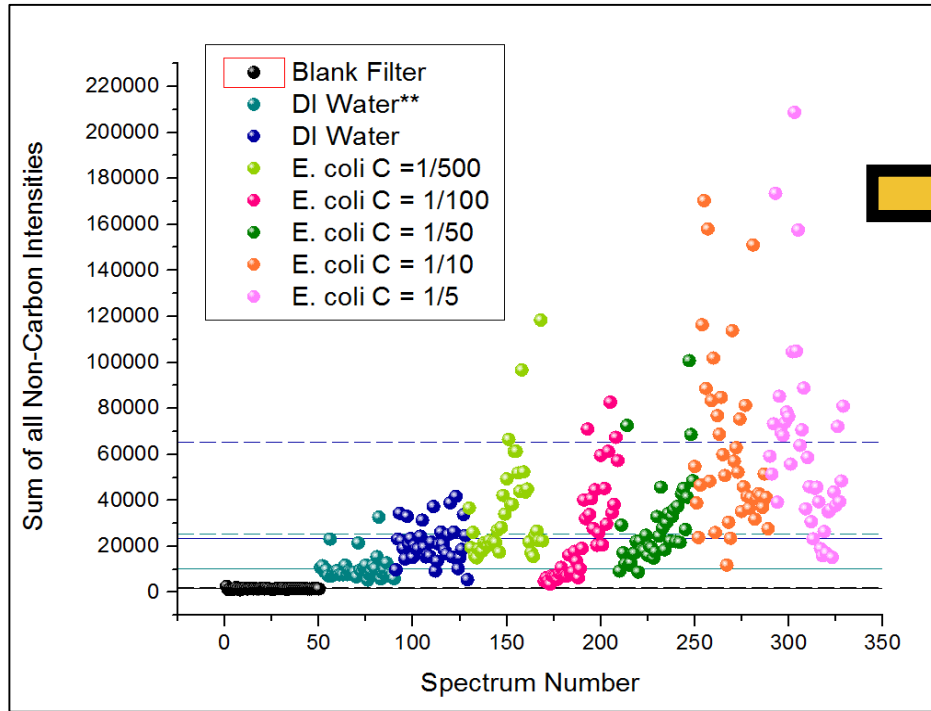

Two separate filters, 20 shots / filter
(all single shot spectra).

Summing intensities of spectral lines.



The people who did the work...



NSERC Discovery Grant



Natural Sciences and Engineering
Research Council of Canada

Conseil de recherches en sciences
naturelles et en génie du Canada

CFI-LOF grant

INNOVATION.CA

CANADA FOUNDATION
FOR INNOVATION

FONDATION CANADIENNE
POUR L'INNOVATION

University of Windsor



University of Windsor



University of Windsor






Thank you!



University of Windsor

Using filters, a better way: the centrifuge insert



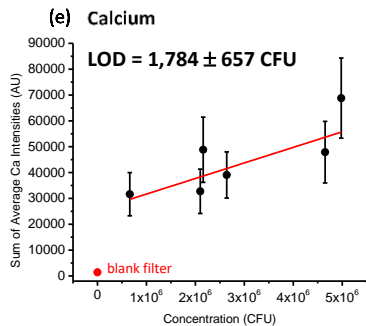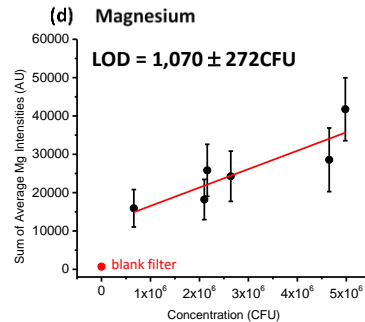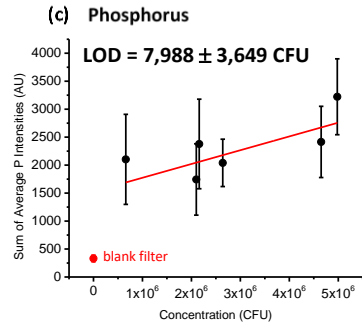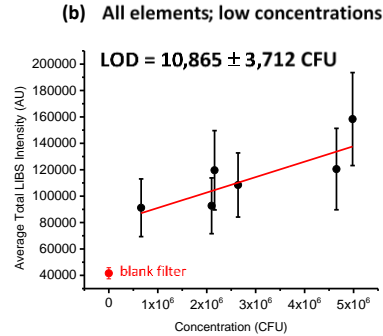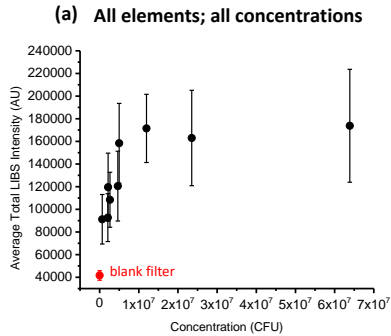

A calibration curve constructed from forty spectra obtained from each of the nine different concentrations returned a LIBS bacterial limit of detection of $10,865 \pm 3,712$ CFU per laser ablation event for bacteria deposited on filters using the metal cone. Limits of detection calculated using only certain elements observed in the LIBS spectra and present in very low concentrations in the filter were even lower: $1,070 \pm 272$ CFU for magnesium and $1,784 \pm 657$ CFU for calcium. This represents a factor of 50 reduction in the limit of detection compared to our previously reported value.



Bacterial LOD

Tungsten powder, average particle size of 12 μm , was used to simulate a contaminant. Tungsten powder was chosen for its inertness, cost and availability, safety of use, ease of preparation, biologically relevant size, and elemental purity. Tungsten powder was added to a suspension of *E. coli*, vortexed, and ~ 0.1 mL was pipetted into the top of the insert prior to centrifugation.


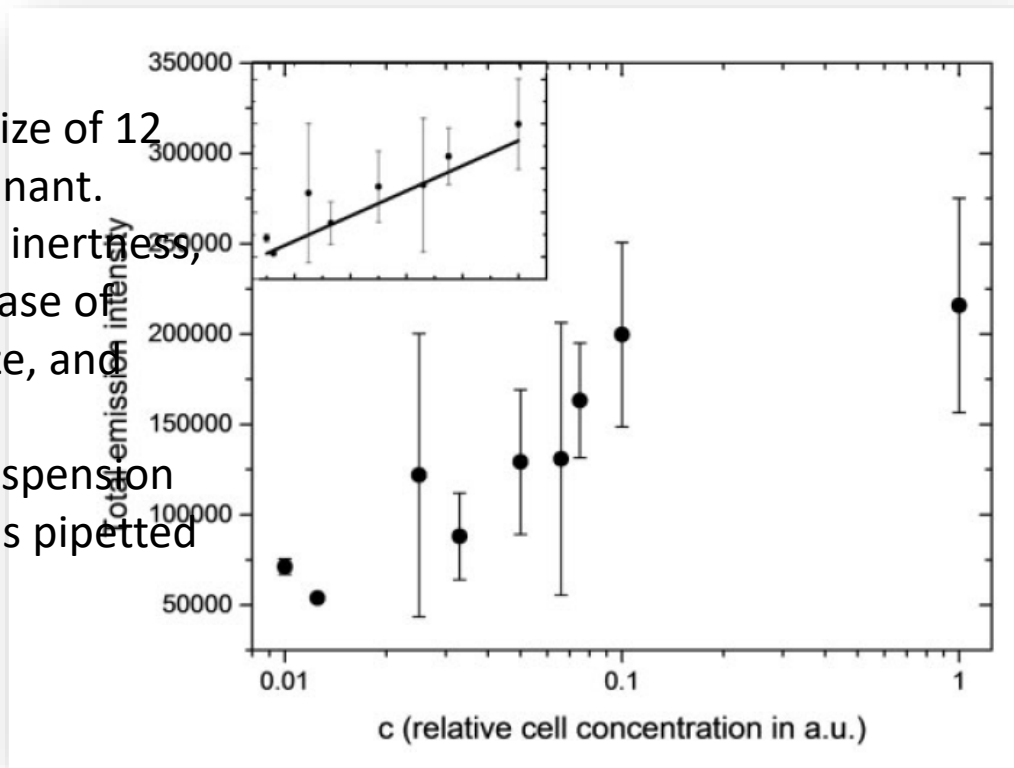



Figure 6. A log-lin calibration curve for bacterial samples. A concentration of $c = 1$ corresponded to 10^{11} cells/mL as determined by optical densitometry resulting in approximately 10^6 cells per ablation. This was the concentration achieved by transferring 24 h of growth for *E. coli* from a TSA plate to 1.5 mL distilled water. The inset shows a linear fit to the lowest eight concentrations on a lin-lin plot.



Typical Bacterial Spectrum

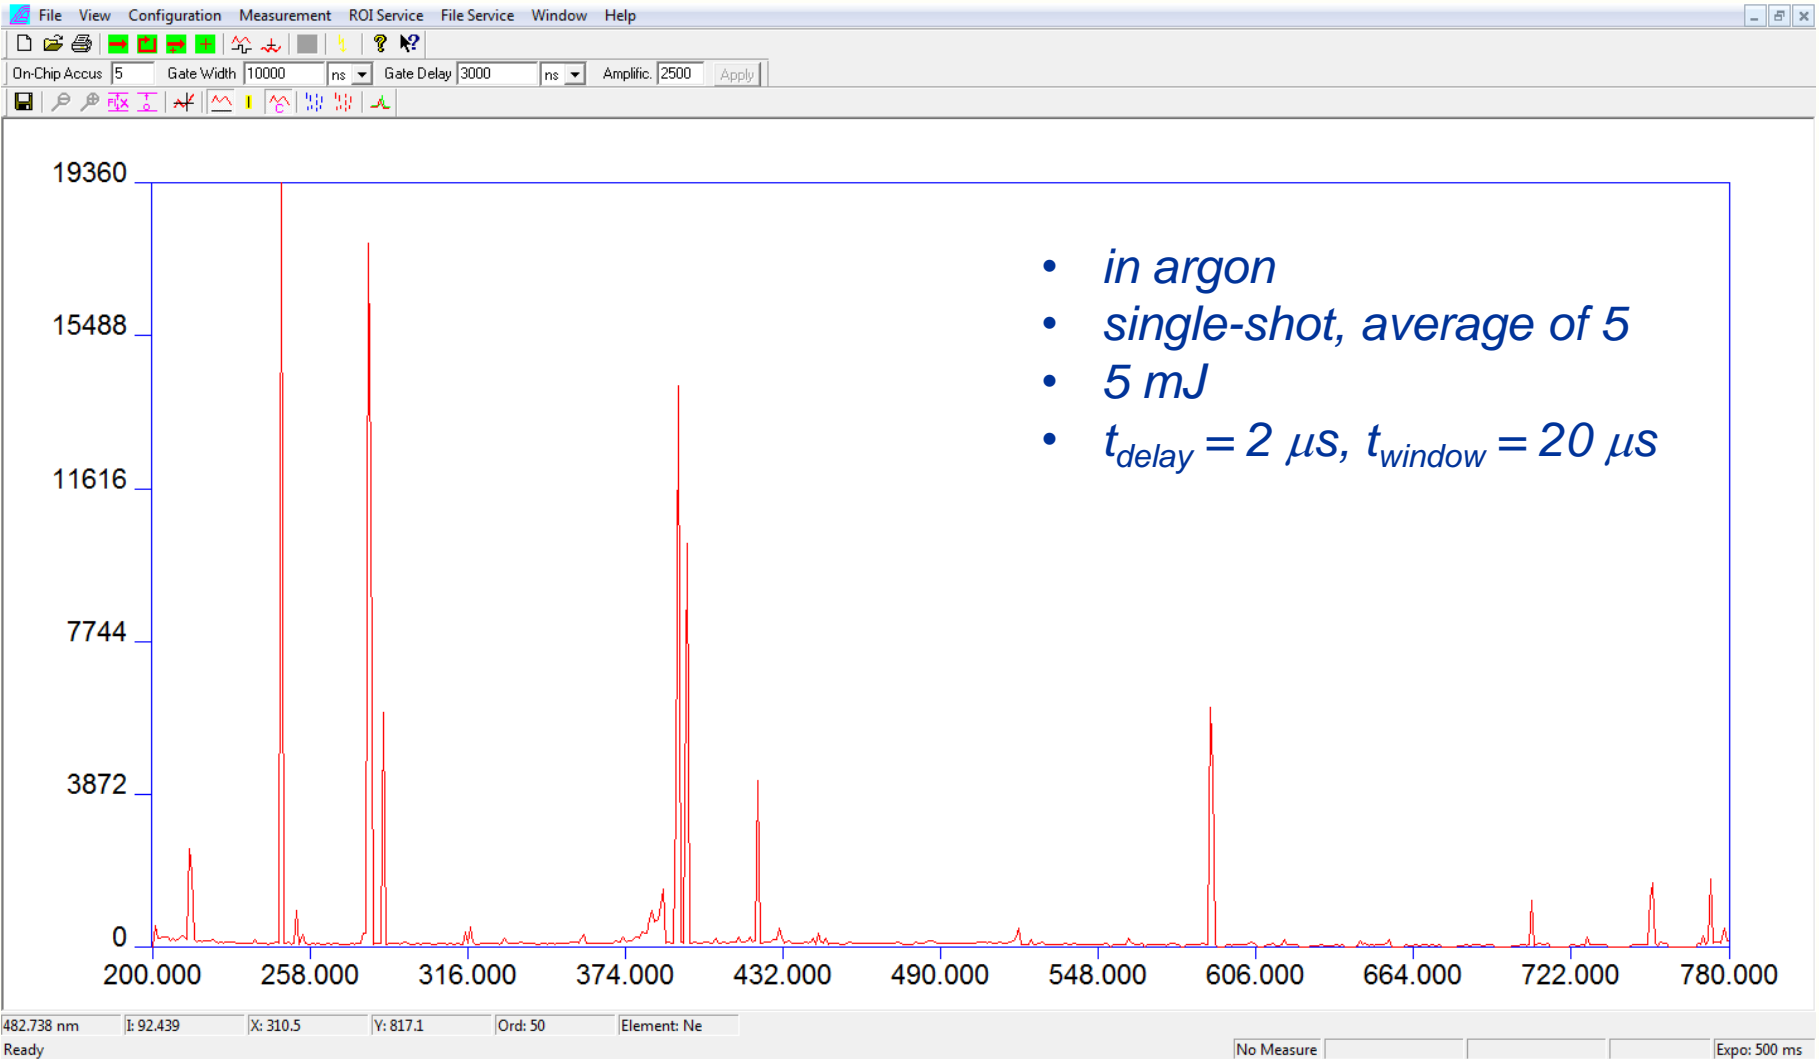


Variable Down-Selection

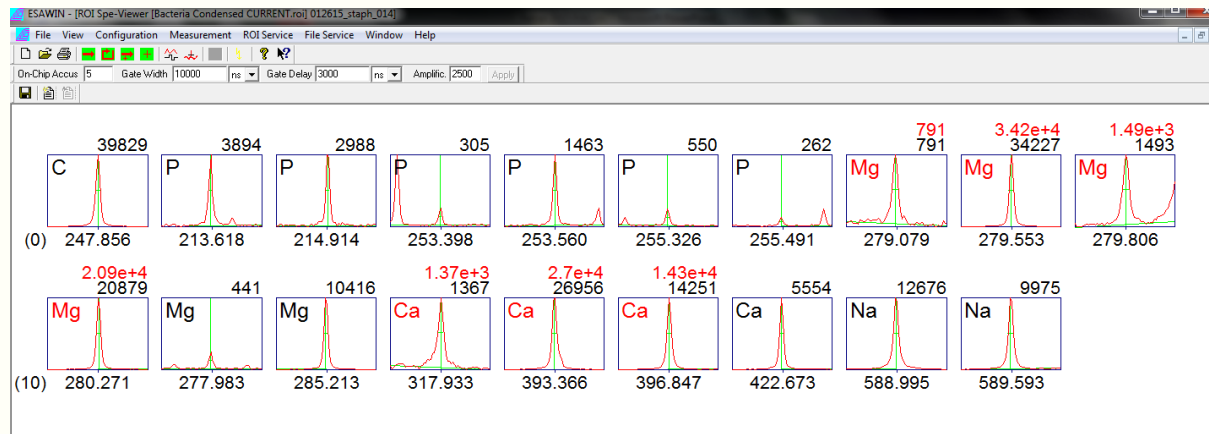

- New classification model
- 164 independent variable
 - 19 line intensities (all divided by sum)
 - 145 ratios of intensities
- No other metals. Beware?
 - Farooq (2014) sees S, Cl, Mn, Fe, Al, Cu, etc.
 - Sivakumar (2015) only sees Ca, Na, Mg, K, O, H, C, P
 - We see Ni, Fe, Ti only when contaminated!

Performance With New Library

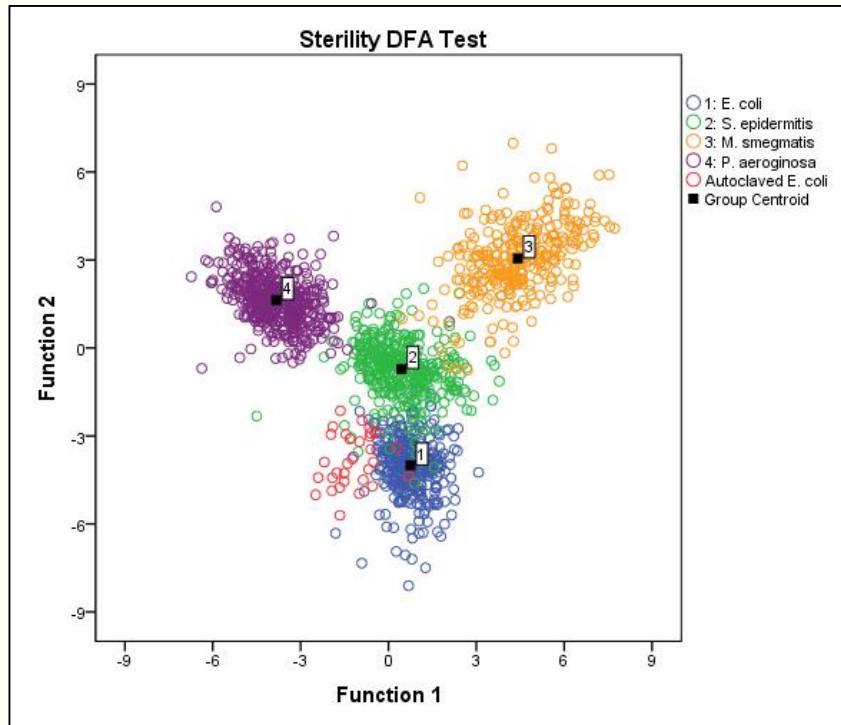

DFA Classification Grouped by Species

<i>Escherichia</i>	TRUE	FALSE	<i>Staphylococcus</i>	TRUE	FALSE
Positive	98.28%	0.77%	Positive	97.75%	1.44%
Negative	99.23%	1.72%	Negative	98.56%	2.25%
<i>Mycobacterium</i>	TRUE	FALSE	<i>Pseudomonas</i>	TRUE	FALSE
Positive	95.36%	0.33%	Positive	99.57%	0.22%
Negative	99.67%	4.64%	Negative	99.78%	0.43%

Sensitivity: $98 \pm 2\%$ Specificity: $99 \pm 1\%$

PLS-DA Classification Grouped by Species

<i>Escherichia</i>	TRUE	FALSE	<i>Staphylococcus</i>	TRUE	FALSE
Positive	96.55%	1.12%	Positive	96.75%	1.53%
Negative	98.88%	3.45%	Negative	98.47%	3.25%
<i>Mycobacterium</i>	TRUE	FALSE	<i>Pseudomonas</i>	TRUE	FALSE
Positive	97.02%	0.41%	Positive	98.92%	0.33%
Negative	99.59%	2.98%	Negative	99.67%	1.08%



Sensitivity: $97 \pm 3\%$ Specificity: $99 \pm 2\%$

All external validation results


	DFA (by filter)	DFA (by species) above	PLSDA (by species) above
Sensitivity	0.93 ± 0.07	0.98 ± 0.02	0.97 ± 0.03
Specificity	0.98 ± 0.03	0.99 ± 0.01	0.99 ± 0.02

“by filter” means approximately 30 groups in DFA, no relationships between groups assumed

New Concentration Study

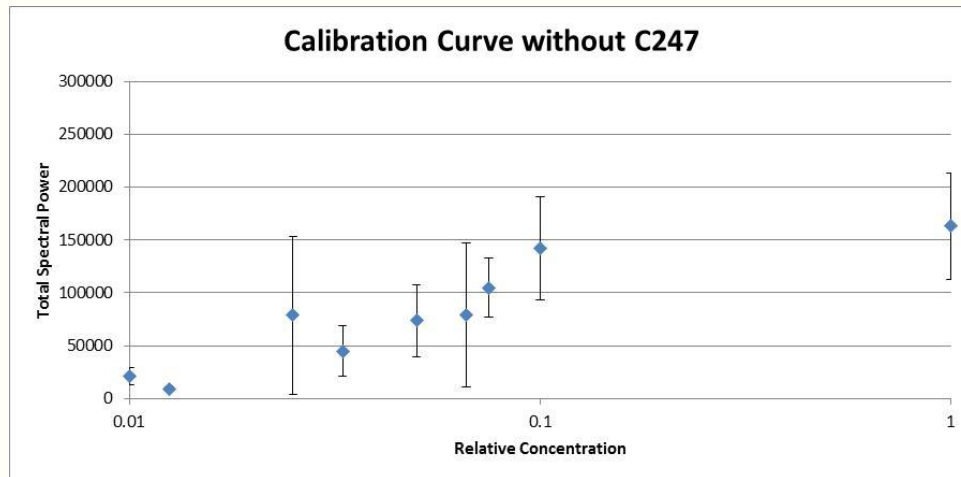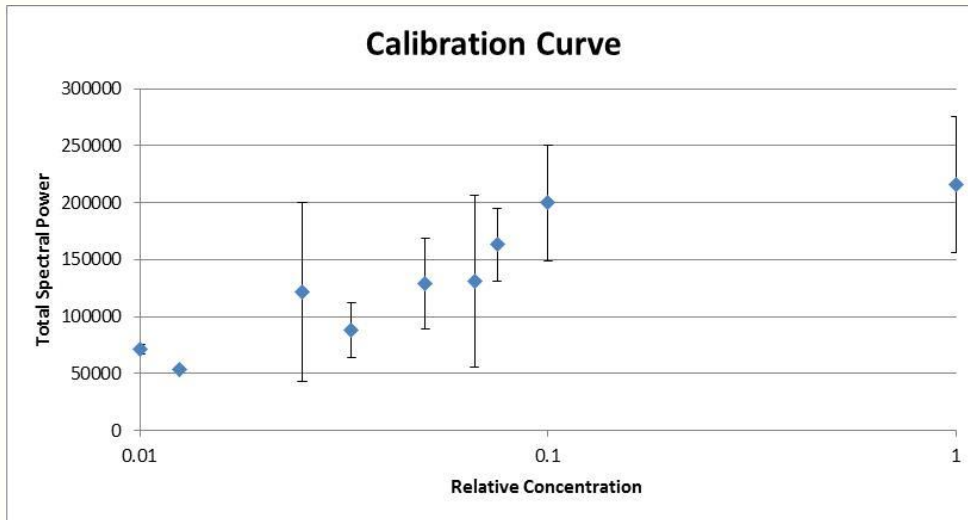


Previous result

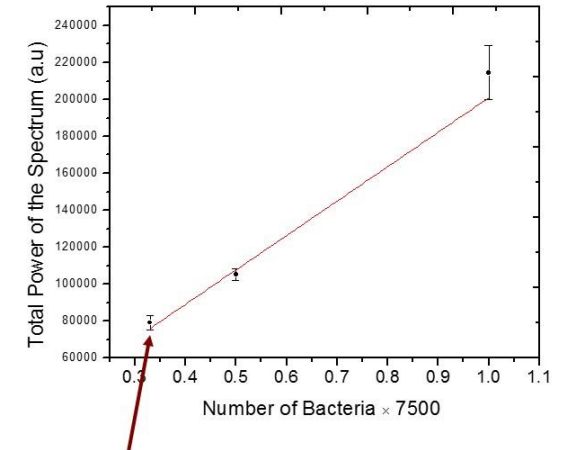

5 laser sampling locations

~500 bacteria per locations



- Performed with serial dilutions.
- “Concentration 1” → harvest entire plate of colonies off TSA, suspend in 1.5 mL distilled H₂O
- Measure with optical densitometry
- OD=0.1 measured for C=0.001 (from literature OD 0.1=10⁸ cells/mL).
- C=1 → 10¹¹ cells/mL
- Implies for C=1, 10⁶/shot

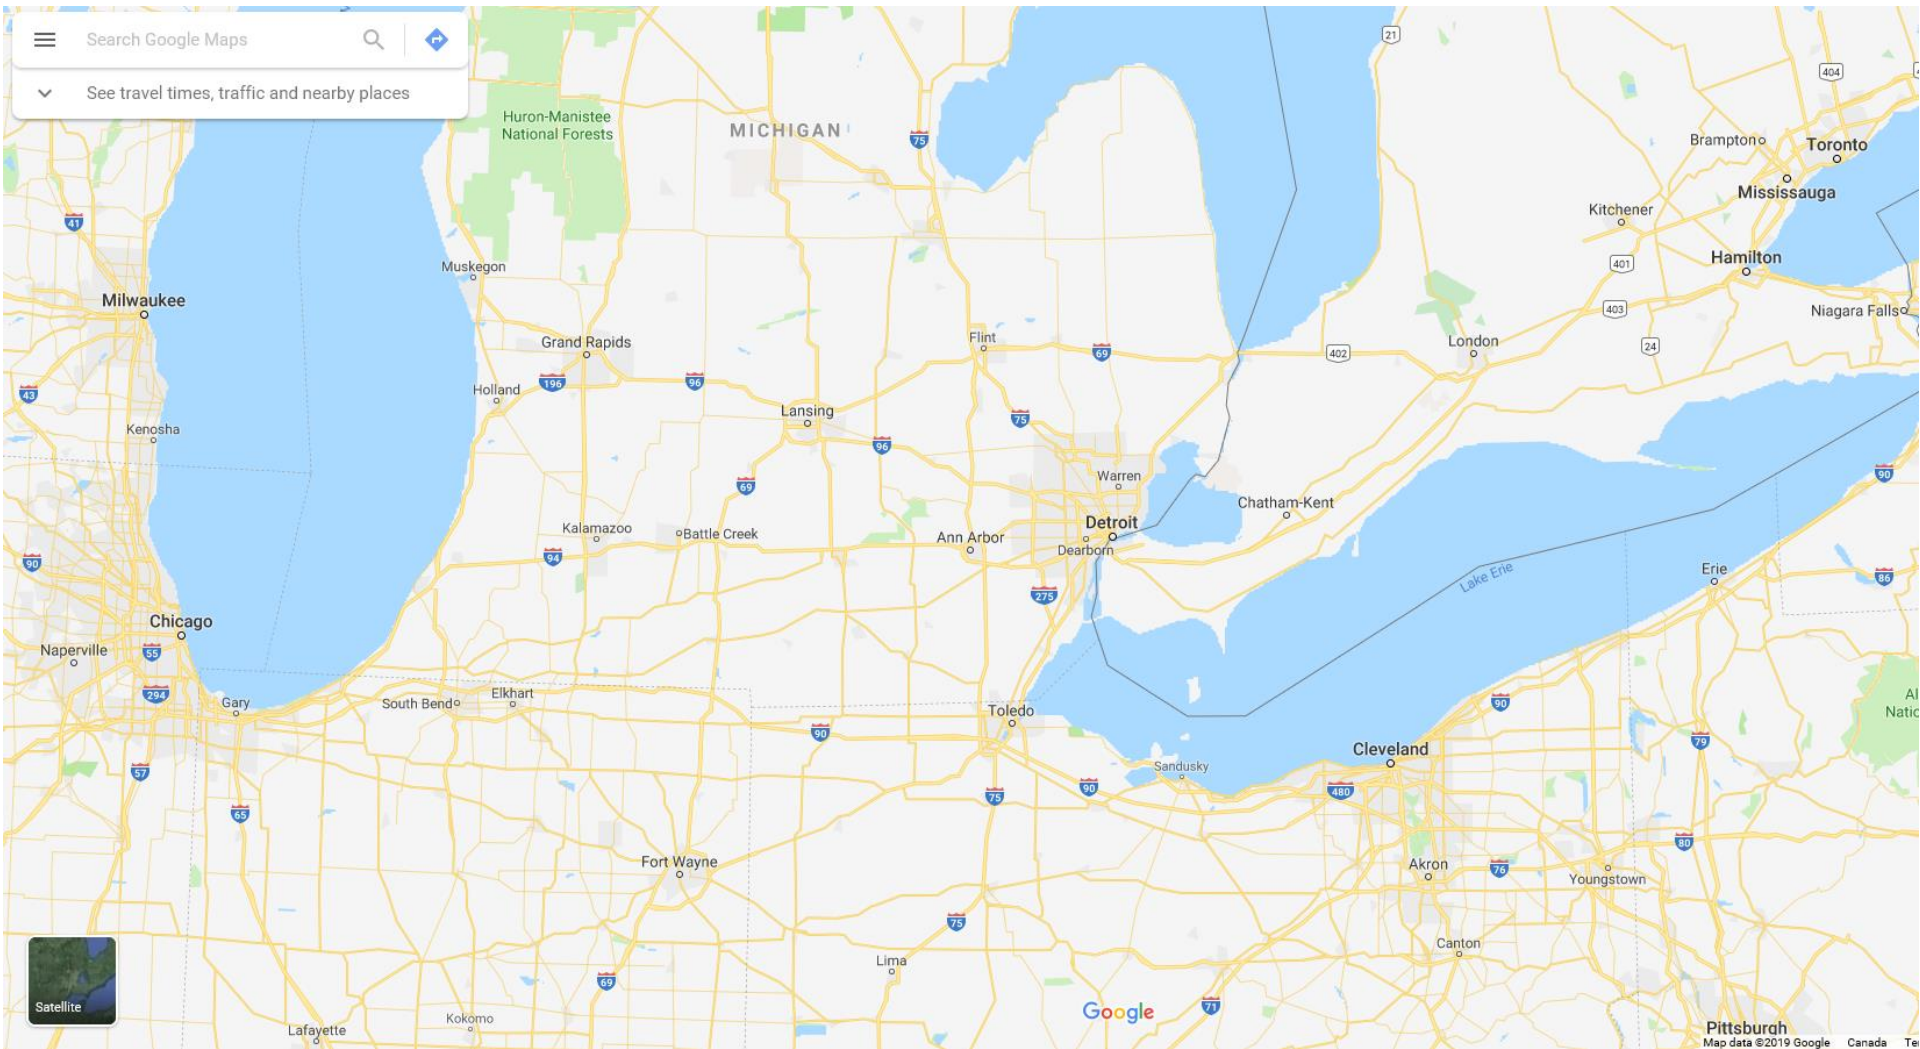

University of Windsor

How unique is “unique”?

- ✓ We can identify a bacterial species, certainly its genus, with high sensitivity and specificity (confirmed by others).
- ✓ We can differentiate strains of *E. coli* (demonstrated by others in MRSA).
- ✓ Multiple multivariate techniques effective at discriminating spectra.

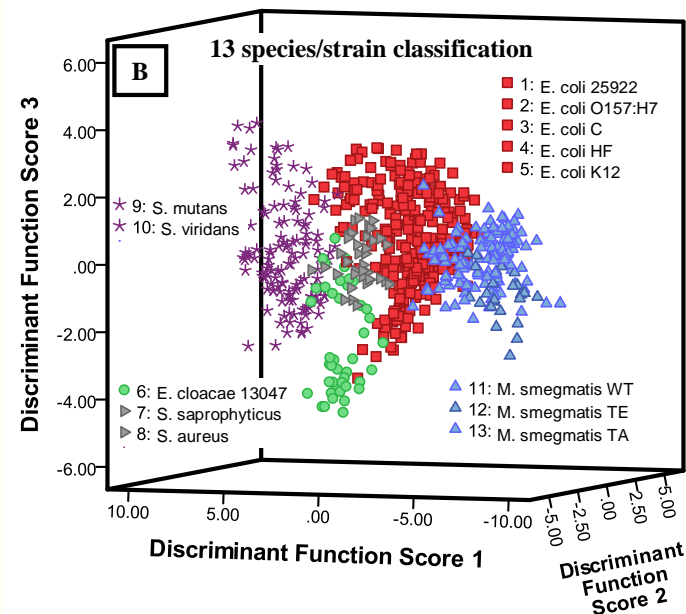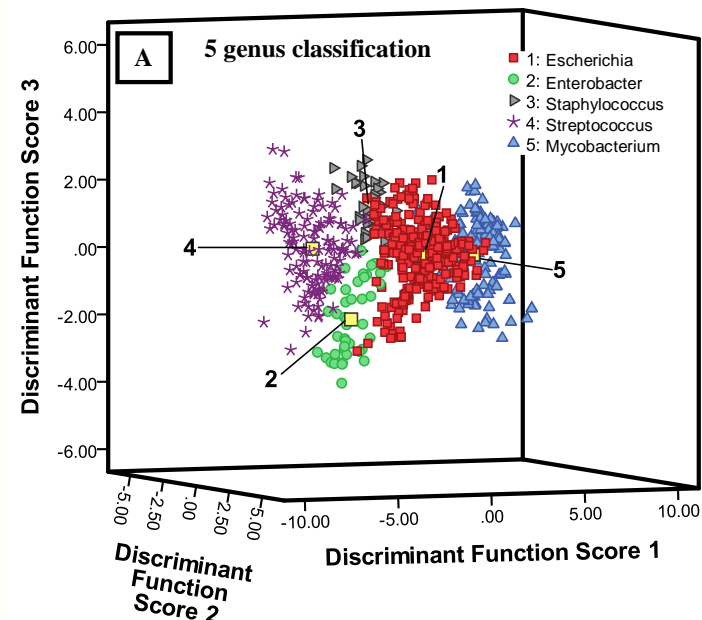


PLSDA

<i>E. COLI</i>	True	False
Positive	95.65%	9.17%
Negative	90.83%	4.35%
<i>STAPHYLOCOCCUS</i>	True	False
Positive	54.05%	0.51%
Negative	99.49%	45.95%
<i>STREPTOCOCCUS</i>	True	False
Positive	95.59%	1.02%
Negative	98.98%	4.41%
<i>MYCOBACTERIUM</i>	True	False
Positive	88.31%	1.06%
Negative	98.94%	11.69%

DFA

<i>E. COLI</i>	True	False
Positive	89.63%	15.95%
Negative	84.05%	10.37%
<i>STAPHYLOCOCCUS</i>	True	False
Positive	86.49%	5.85%
Negative	94.15%	13.51%
<i>STREPTOCOCCUS</i>	True	False
Positive	99.26%	13.32%
Negative	88.68%	0.74%
<i>MYCOBACTERIUM</i>	True	False
Positive	96.10%	4.08%
Negative	95.92%	3.90%

DFA: Sensitivity: $91.37 \pm 16.39 \%$ Specificity: $97.46 \pm 9.35 \%$
PLSDA: Sensitivity: $93.13 \pm 10.25 \%$ Specificity: $90.60 \pm 21.33 \%$

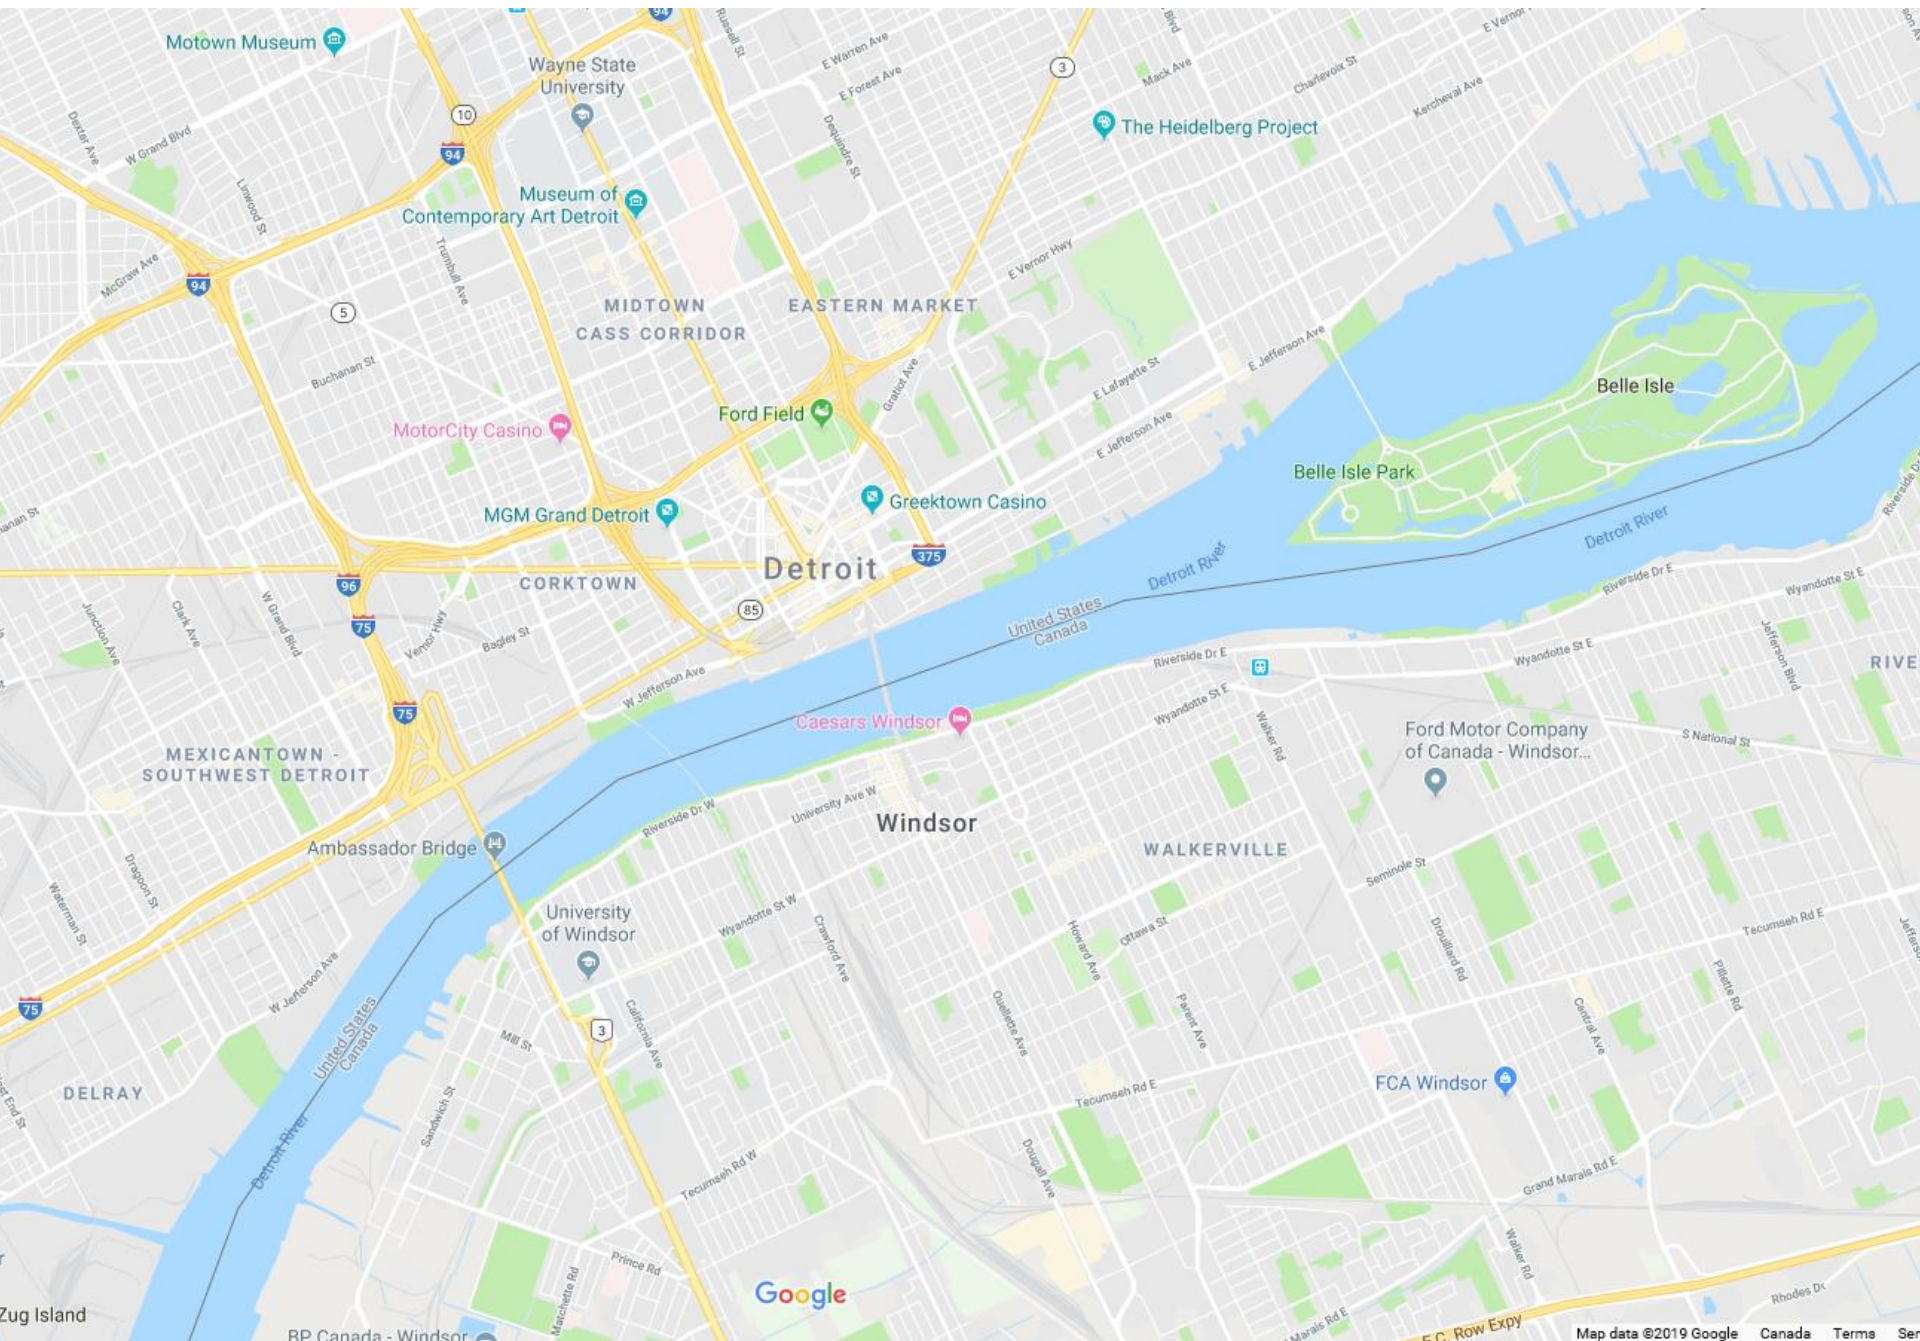

Google

